

Create it 

TIP GUIDE

ULTRASONIC BONE
SURGERY



NSK

SURG

- BONE SURGERY P03-P10
- BONE SURGERY (MAXI REACH) P11-P14
- SCRAPER P15-P16
- EXTRACTION P17-P18
- SOCKET LIFT (CRESTAL APPROACH) P19-P22
 - IMPLANT PREPARATION P23-P26
 - SOCKET LIFT (CRESTAL APPROACH) P27-P28*
 - SINUS LIFT P29
 - SINUS MEMBRANE DETACHMENT P30

PERIO

- SCALING P31-P33
- PERIO P34
- PERIO-CONTROL P35-P36

ENDO

- ENDODONTICS P37-P38
- TIP KIT P39-P42


*Pictures provided by Yasuhiro Kizu, D.D.S., Ph.D.
OMFC (ORAL & MAXILLOFACIAL CARE CLINIC YOKOHAMA)

VARIOSURG TIP LINEUP

- SURG** SURG mode for bone surgery
- PERIO** PERIO mode for maintenance
- ENDO** ENDO mode for root canal treatment



The tips are designed to preserve tissue, maintain cutting speed and easily cut into bone. Saw like teeth on an uneven blade edge enhances bone cutting. This also reduces clogging to maintain cutting speed.

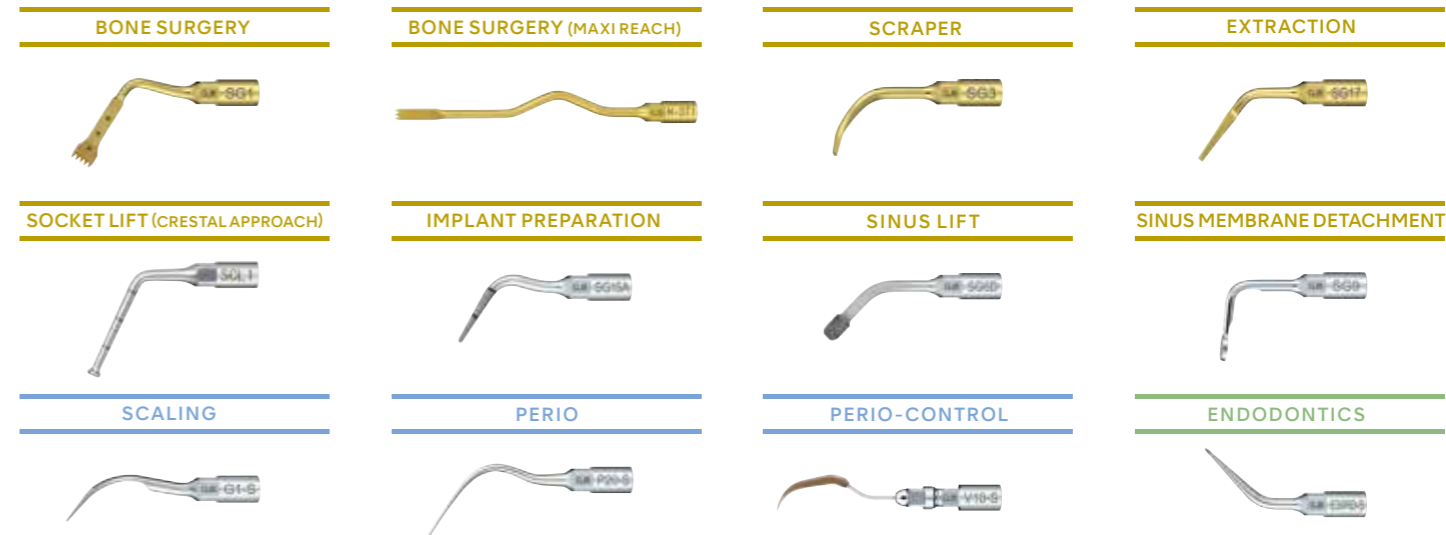

Washable in the Thermodisinfectant

Autoclavable

HIGH POWER Tips that correspond to high power can be used up to 150% power setting.




BONE SURGERY

BONE SURGERY

For chin bone harvests, notably for the mental foramen and mandibular ramus. For general bone surgery.

MODEL **SG1** POWER LEVEL **SURG** 80%

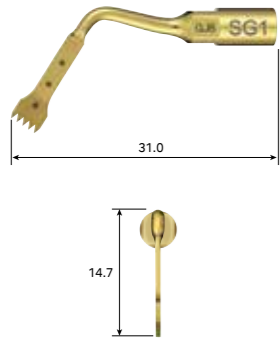


ORDER CODE
Z305101

- TiN coating • Dots mark 3, 6 and 9 mm from tip end
- Five teeth; 0.6 mm thick

MODEL **H-SG1** POWER LEVEL **SURG** 150%

HIGH POWER

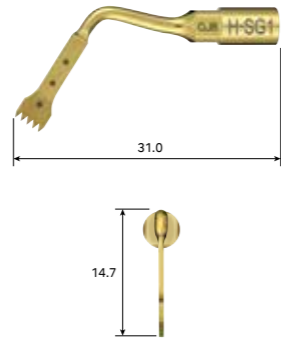


ORDER CODE
Z305151

- TiN coating • Dots mark 3, 6 and 9 mm from tip end
- Five teeth; 0.6 mm thick

MODEL **SG1A** POWER LEVEL **SURG** 80%


For use in deeper regions requiring longer tips.

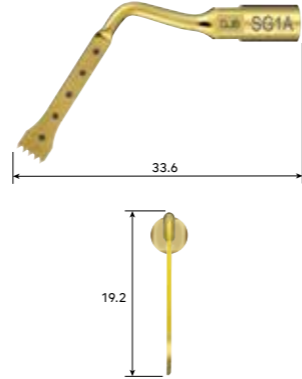

ORDER CODE
Z305138

- TiN coating • Dots mark 3, 6, 9, 12 and 15 mm from tip end
- Five teeth; 0.6 mm thick

MODEL **SG8** POWER LEVEL **SURG** 80%

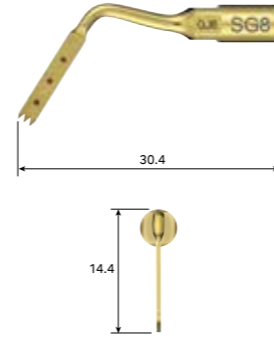


ORDER CODE
Z305109

- TiN coating • Dots mark 3, 6 and 9 mm from tip end
- Three teeth; 0.6 mm thick

MODEL **H-SG8** POWER LEVEL **SURG** 150%

HIGH POWER

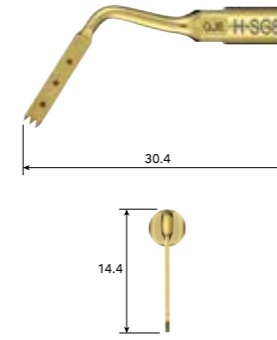


ORDER CODE
Z305155

- TiN coating • Dots mark 3, 6 and 9 mm from tip end
- Three teeth; 0.6 mm thick

MODEL **SG8A** POWER LEVEL **SURG** 80%

For use in deeper regions requiring longer tips.

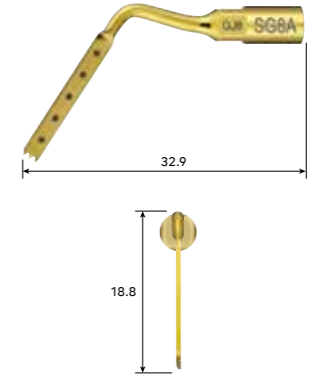

ORDER CODE
Z305139

- TiN coating • Dots mark 3, 6, 9, 12 and 15 mm from tip end
- Three teeth; 0.6 mm thick





Unilateral anterior mandibular sampling
SG1, H-SG1, SG1A

BONE SURGERY

For harvesting bone from the mandibular ramus.

MODEL **SG12** POWER LEVEL **SURG** 100%


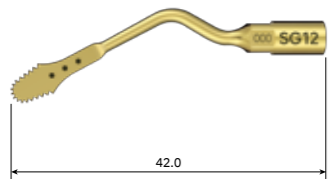


ORDER CODE

ZT02010001

- TiN coating • Dots mark 6, 8 and 10 mm from tip end
- Eighteen teeth; 0.35 mm thick

MODEL **SG14R** POWER LEVEL **SURG** 80%





ORDER CODE

Z305122

- TiN coating • 90 degree right curved tip*
- Five teeth; 0.6 mm thick

MODEL **SG14L** POWER LEVEL **SURG** 80%



ORDER CODE

Z305123

- TiN coating • 90 degree left curved tip*
- Five teeth; 0.6 mm thick



Anterior mandibular harvesting
SG14R, SG14L


* The direction of the tip's curve is defined by the tip's anterior view.

BONE SURGERY

For harvesting bone from the mandibular ramus.

MODEL **H-SG8R** POWER LEVEL **SURG** 150%

HIGH POWER




ORDER CODE

Z305156

- TiN coating • 90 degree right curved tip*
- Three teeth; 0.6 mm thick

MODEL **H-SG8L** POWER LEVEL **SURG** 150%

HIGH POWER



ORDER CODE

Z305157



- TiN coating • 90 degree left curved tip*
- Three teeth; 0.6 mm thick

* The direction of the tip's curve is defined by the tip's anterior view.

BONE SURGERY

For excisions in areas with inclines or projections or which are otherwise hard to access with SG1 and other regular tips.

MODEL **SG2R** POWER LEVEL **SURG** 80%





ORDER CODE
Z305102

- TiN coating • Right curved tip*
- Three teeth; 0.6 mm thick



Excision of bone torus
SG2R, SG2L

MODEL **SG2L** POWER LEVEL **SURG** 80%




ORDER CODE
Z305103

- TiN coating • Left curved tip*
- Three teeth; 0.6 mm thick

MODEL **SG19** POWER LEVEL **SURG** 80%

For cutting curved surfaces.



ORDER CODE
Z305135

- TiN coating • Dot mark 3 mm from tip end
- Five teeth; 0.8 mm thick




Mandibular harvesting at approach stage
SG19

For regions that are hard to access with regular tips, notably the posterior mandible or curved areas.

BONE SURGERY

MODEL **SG30** POWER LEVEL **SURG** 50%

For narrow cutting to reduce bone loss. Also suitable for corticotomies.



ORDER CODE
Z305137


- TiN coating • Sharp edge • 0.5 mm thick



Alveolar crestal incision for harvesting bone (when narrowing bone cuts)
SG30

MODEL **SG58** POWER LEVEL **SURG** 80%

For removing tori on the posterior mandible or mandibular lingual surface.

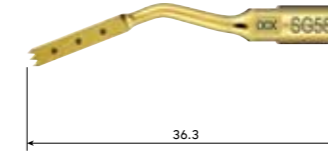


ORDER CODE
Z305141

- TiN coating • Dots mark 3, 6 and 9 mm from tip end
- Three teeth; 0.6 mm thick



The cutting part is bone torus
SG58

MODEL **SG68** POWER LEVEL **SURG** 80%

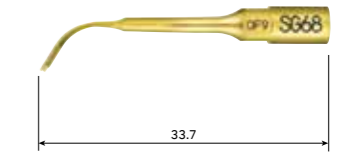


ORDER CODE
Z305143

- TiN coating • Marking every 2 and 4 mm from top of tip (Single side)
- Three teeth; 0.6 mm thick



Vertical osteotomy for harvesting bone
SG68

* The direction of the tip's curve is defined by the tip's anterior view.

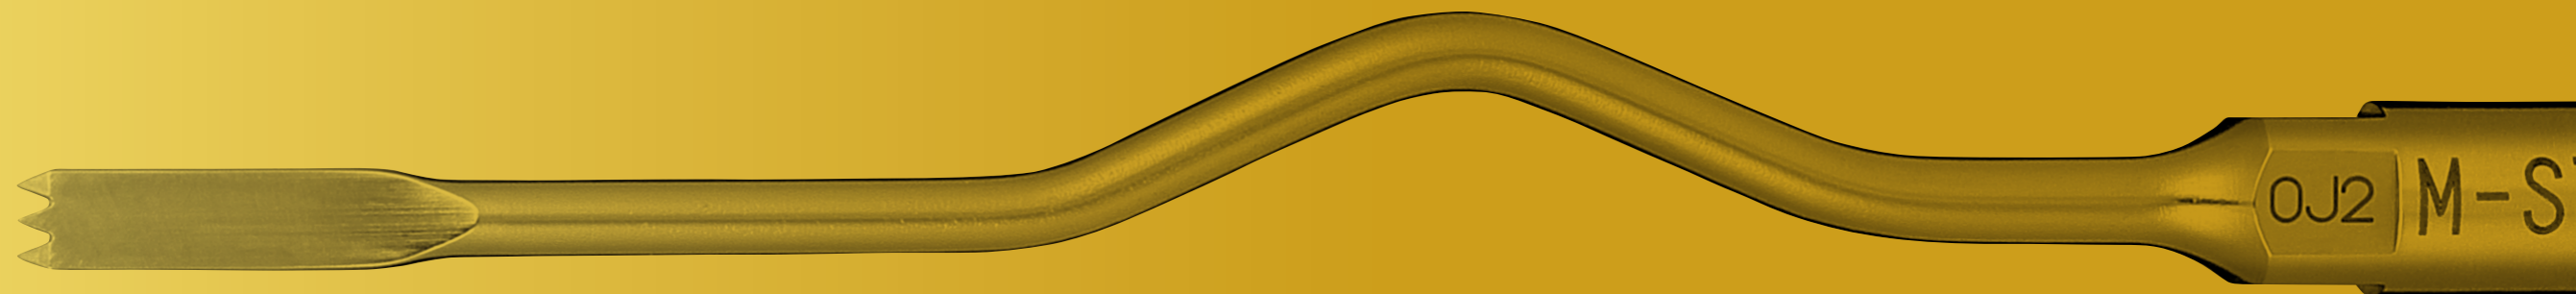

**BONE SURGERY
(MAXI REACH)**

BONE SURGERY (MAXI REACH)


MODEL **M-RE2** POWER LEVEL **SURG** 80%




ORDER CODE

Z305715

- TiN coating • Eleven teeth
- 0.6 mm thick




Mandibular ramus SSRO
Horizontal osteotomy lines on the medial aspect.



Le Fort type I osteotomy
Trimming near the descending palatine artery.


MODEL **M-ST1** POWER LEVEL **SURG** 80%



ORDER CODE

Z305713



- TiN coating • Three teeth
- 0.6 mm thick



Mandibular ramus SSRO
Separation of cortical and maritime bone during sagittal division.

BONE SURGERY (MAXI REACH)


MODEL **M-OC1R** POWER LEVEL **SURG** 80%



ORDER CODE


Z305709

- TiN coating • Dots mark 2 mm from tip end • Right curved tip*
- 3 teeth; 0.6 mm thick



Le Fort type I osteotomy
Pterygomaxillary junction dissection.

MODEL **M-OC1L** POWER LEVEL **SURG** 80%



ORDER CODE

Z305710

- TiN coating • Dots mark 2 mm from tip end • Left curved tip*
- 3 teeth; 0.6 mm thick



Mandibular branch vertical osteotomy (IVRO)
Assignment of starting point and guide grooves.

* The direction of the tip's curve is defined by the tip's anterior view.

SCRAPER



For flattening the alveolar crest or harvesting bone fragments. **SCRAPER**

MODEL **SG3**







POWER LEVEL **SURG** 80%

MODEL **SG4**

POWER LEVEL **SURG** 80%

MODEL **SG5**

POWER LEVEL **SURG** 80%



ORDER CODE

Z305104

ORDER CODE

Z305105

ORDER CODE

Z305106

- TiN coating • Triple sided edge spatula tip
- Single-edged scraper

- TiN coating • Edge spatula tip
- Double-edged scraper

- TiN coating • Rounded edge spatula tip
- Single-edged scraper



Alveolar crest flattening
SG3



Osteoplasties
SG5



EXTRACTION

Ruptures the periodontal ligament to streamline suture removal. Also effective in extracting ankylosed teeth.

EXTRACTION

MODEL **SG17**



POWER LEVEL **SURG** 80%

MODEL **SG18R**

POWER LEVEL **SURG** 50%

MODEL **SG18L**



POWER LEVEL **SURG** 50%



ORDER CODE

Z305132



• TiN coating • 0.7 mm thick



ORDER CODE

Z305133

• TiN coating • Right angled tip* • 0.7 mm thick



ORDER CODE


Z305134

• TiN coating • Left angled tip* • 0.7 mm thick



Extraction
SG17, SG18R, SG18L


*The direction of the tip's angle is defined by the tip's anterior view.

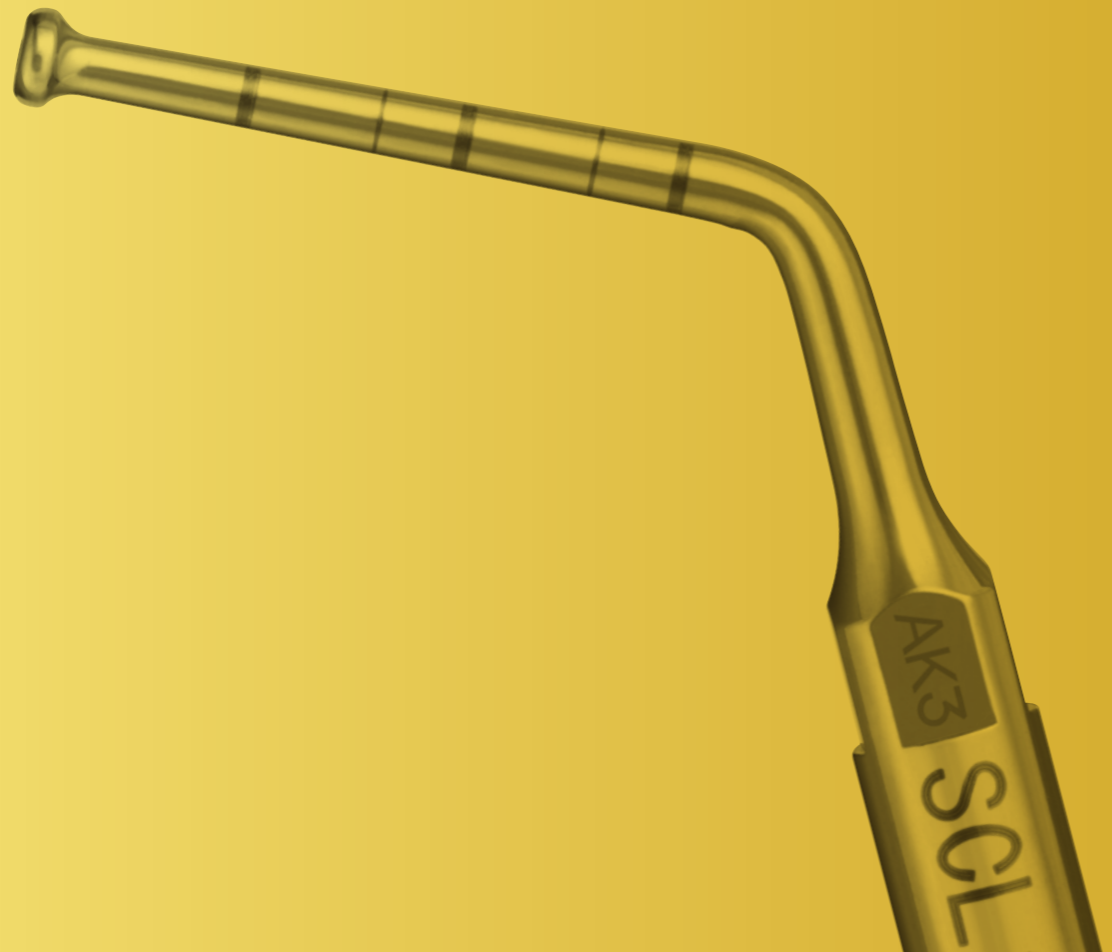

SOCKET LIFT
(CRESTAL APPROACH)

SOCKET LIFT (CRESTAL APPROACH) Socket lift procedures.


The socket lift tip enhances the safety of procedures, being less invasive and enabling sinus lifts with short chair times.
 Osteotomy with ultrasonic vibration reduces the risk of damage to the Schneiderian membrane.
 Eliminating hammering taps through the osteotome technique reduces patient discomfort and potential dizziness.

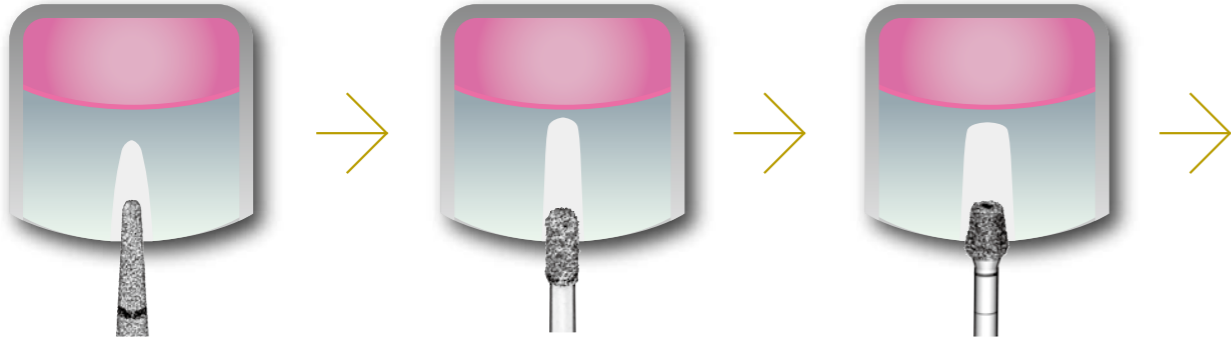

A starting point is added to trigger bone formation.

Bone formation to prepare implant site.

Implant site expansion and formation.

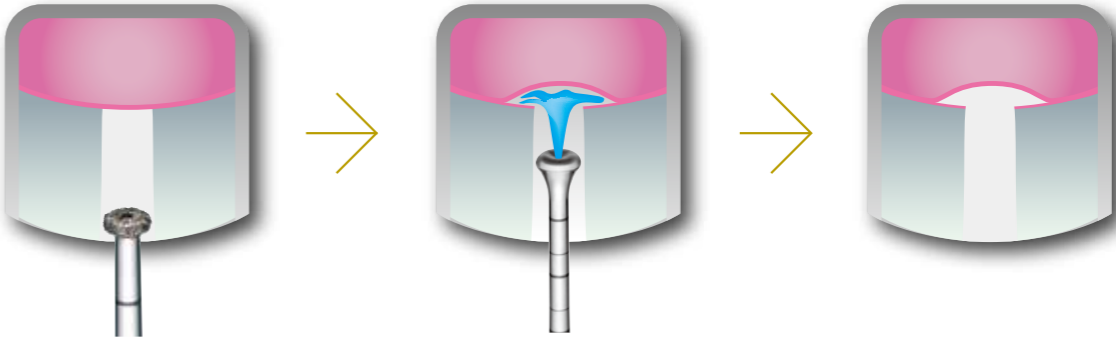

Maxillary sinus perforation and bone formation on alveolar ridge.

Reliably elevate the maxillary sinus membrane with internal irrigation.




Forms implant preparation site once maxillary sinus membrane is elevated.

IMPLANT PREPARATION

For preparation of implant sites, adding starting points, and other steps.

MODEL **SG15A** POWER LEVEL **SURG** 50%

MODEL **SG15B** POWER LEVEL **SURG** 50%

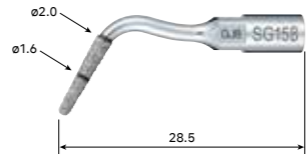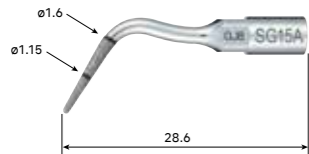

ORDER CODE

Z305124

ORDER CODE

Z305125

- Diamond coating • Tip-end diameter; 0.7 mm
- Markings every 5 mm and 10 mm from tip end

- Diamond coating • Tip-end diameter; 1.3 mm
- Markings every 5 mm and 10 mm from tip end



Implant preparation
SG15A, SG15B






IMPLANT PREPARATION

For preparation of implant sites, flattening bone surfaces, and other steps.

MODEL **SG15C** POWER LEVEL **SURG** 50%

MODEL **SG15D** POWER LEVEL **SURG** 50%

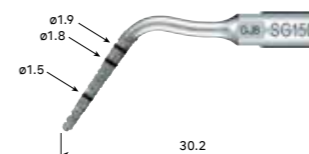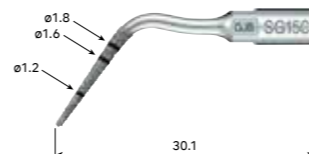

ORDER CODE

Z305126

ORDER CODE

Z305127

- Diamond coating • Tip-end diameter; 0.9 mm
- Markings every 5 mm, 10 mm and 12 mm from tip end

- Diamond coating • Tip-end diameter; 1.3 mm
- Marking every 5 mm, 10 mm and 12 mm from tip end




Implant preparation
SG15C, SG15D



IMPLANT PREPARATION

For expanding and forming implant preparation site when approaching from the alveolar crest.

MODEL **SG16A** POWER LEVEL **SURG** 50%

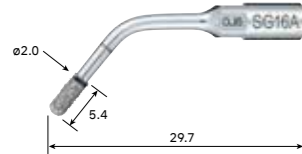

ORDER CODE



Z305128

- Diamond coating • Diameter ; 2.0 mm
- Markings every 5 mm and 10 mm from tip end



Implant preparation
SG16A

MODEL **SG16B** POWER LEVEL **SURG** 50%

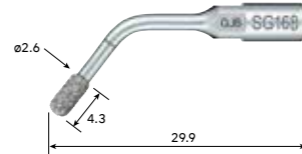

ORDER CODE

Z305129

- Diamond coating • Diameter ; 2.6 mm
- Markings every 5 mm and 10 mm from tip end



Implant preparation
SG16B




For expanding and forming implant preparation site when approaching from the alveolar crest.

IMPLANT PREPARATION

MODEL **SCL2D** POWER LEVEL **SURG** 50%


INTERNAL IRRIGATION



ORDER CODE

Z305182

- Diamond coating





Implant preparation site depth can be measured using markings on the tip.



MODEL **SCL4D** POWER LEVEL **SURG** 80%

INTERNAL IRRIGATION

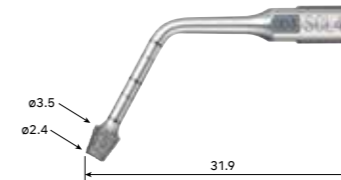

ORDER CODE

Z305184

- Diamond coating



Formation of implant preparation site
SCL2D, SCL4D





SOCKET LIFT (CRESTAL APPROACH)

For procedures such as osteotomy of maxillary sinus approaching from the alveolar crest and implant preparation site adjustments.

MODEL **SCL1D** POWER LEVEL **SURG** 80%

INTERNAL IRRIGATION

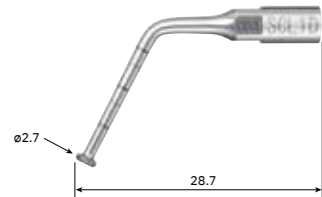



ORDER CODE

Z305171

• Diamond coating

MODEL **SCL3D** POWER LEVEL **SURG** 80%

INTERNAL IRRIGATION

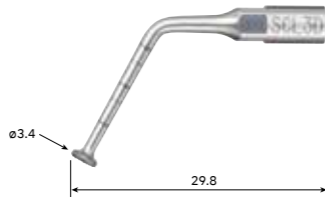



ORDER CODE

Z305173

• Diamond coating

MODEL **SCL5D** POWER LEVEL **SURG** 80%


INTERNAL IRRIGATION

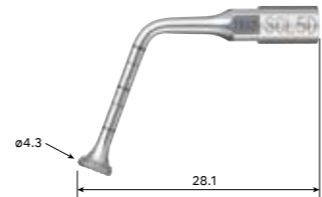

ORDER CODE

Z305175

• Diamond coating



Implant preparation site depth can be measured using markings on the tip.



Cutting the cavity floor of implant preparation site
SCL1D, SCL3D, SCL5D





Elevating the sinus membrane with internal irrigation approaching from alveolar crest.

SOCKET LIFT (CRESTAL APPROACH)

MODEL **SCL1** POWER LEVEL **SURG** 50%

INTERNAL IRRIGATION


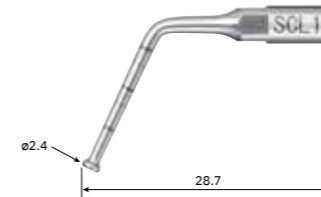


ORDER CODE

Z305170

MODEL **SCL3** POWER LEVEL **SURG** 50%

INTERNAL IRRIGATION


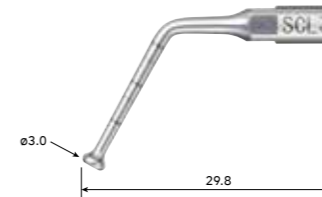


ORDER CODE

Z305172


MODEL **SCL5** POWER LEVEL **SURG** 50%

INTERNAL IRRIGATION

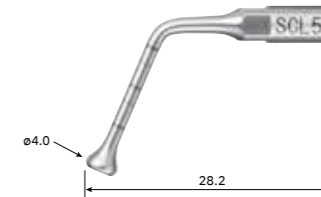

ORDER CODE

Z305174



Implant preparation site depth can be measured using markings on the tip.




Before the mucous membrane of maxillary sinus is elevated
SCL1, SCL3, SCL5



SINUS LIFT

For bone fenestration and bone formations.

MODEL **SG6D** POWER LEVEL **SURG** 80%



ORDER CODE


Z305107

• Diamond coating



Avulsion of wisdom teeth and impacted teeth
SG6D

MODEL **SG7D** POWER LEVEL **SURG** 50%



ORDER CODE

Z305108



• Diamond coating



Lateral maxillary posterior bone augmentation
SG7D

For detachment and elevation of the maxillary sinus membrane. SINUS MEMBRANE DETACHMENT

MODEL **SG9** POWER LEVEL **SURG** 50%



ORDER CODE



Z305110

• Flat circular convex elevator • Angled at 90°



Sinus membrane detachment
SG9, SG10

MODEL **SG10** POWER LEVEL **SURG** 50%




ORDER CODE

Z305111

• Flat circular convex elevator • Angled at 135°


MODEL **SG11** POWER LEVEL **SURG** 50%




ORDER CODE

Z305112

• Cone compressor



Sinus membrane elevation
SG11

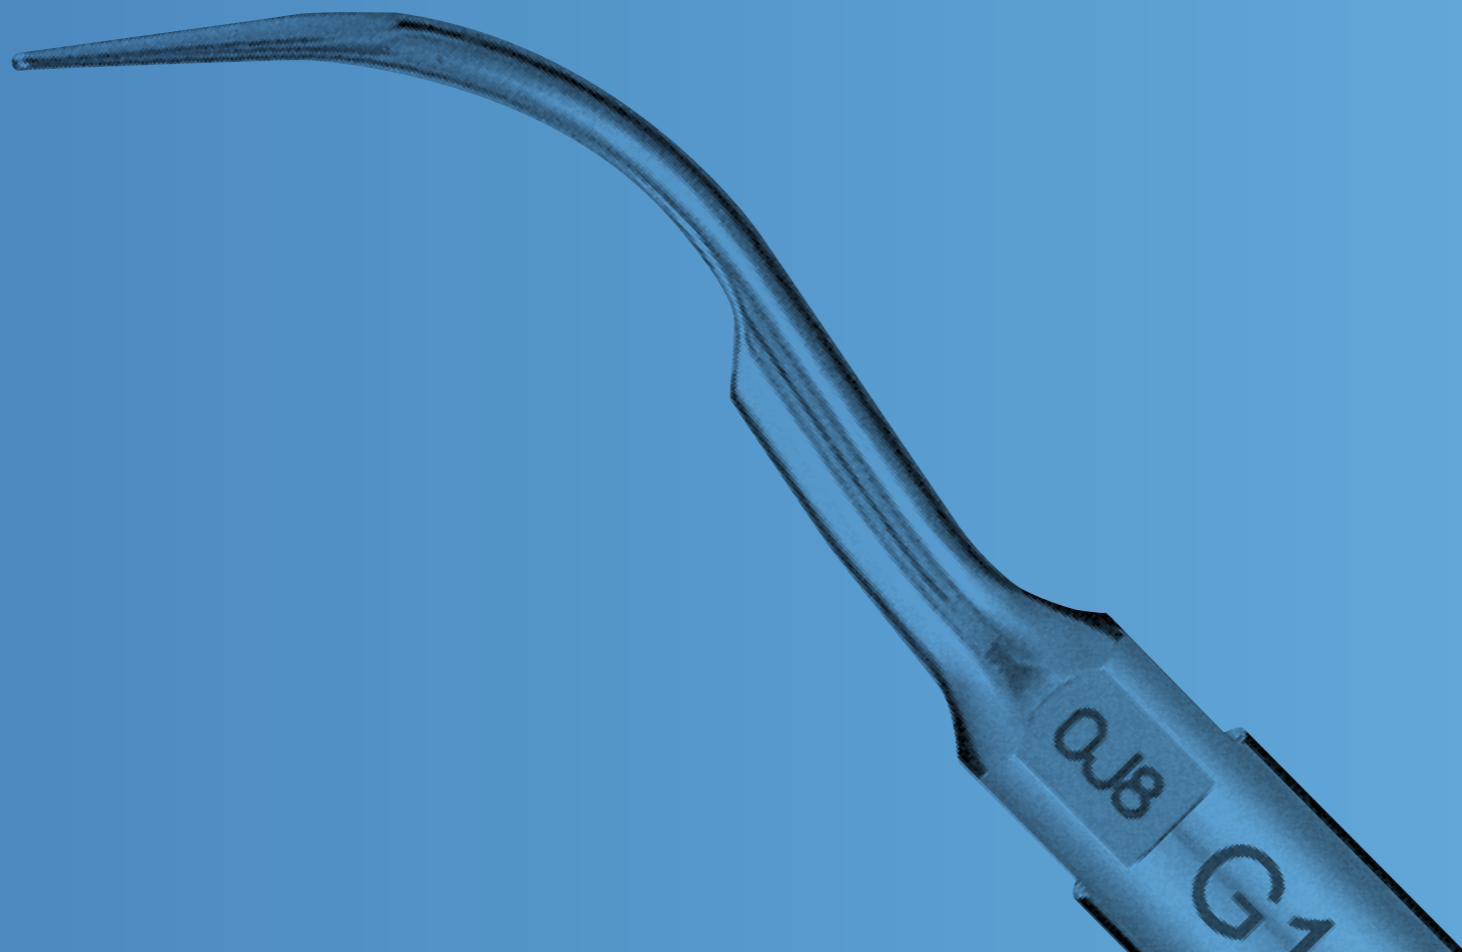


SCALING

SCALING

Removal of supra gingival tartar, tartar narrow interdental space, marginal gingival calculus.

MODEL **G1-S** POWER LEVEL **SURG** 50%



ORDER CODE

Z305113




Single rooted / Multi rooted
G1-S

PERIO

Removal of gingival biofilm.

MODEL **P20-S** POWER LEVEL **PERIO** 100%

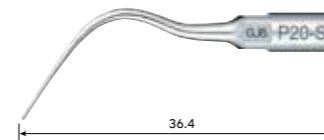

ORDER CODE



Z305114



Single rooted / Multi rooted
P20-S

MODEL **P25R-S** POWER LEVEL **PERIO** 100%

Removal of Biofilm furcation area.

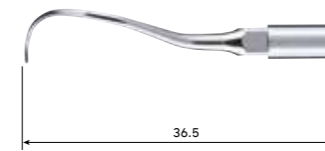

ORDER CODE

Z305115


• Right curved type*



Single rooted / Multi rooted
P25R-S, P25L-S

MODEL **P25L-S** POWER LEVEL **PERIO** 100%

Removal of Biofilm furcation area.



ORDER CODE

Z305116

• Left curved type*


* The direction of the tip's curve is defined by the tip's anterior view.

MODEL **V10-S** POWER LEVEL **PERIO** 100%

MODEL **V-P10**



For the maintenance of prostheses and implants. Produced from special material to allow safe debridement without causing damage to metals and implants.



ORDER CODE
Z305117

- Includes E-Tip replacement wrench
- Plastic Tip is not included



ORDER CODE
Y900184

- Pack of 3
- V10-S holder is not included



V-P10

MODEL **V-P11R**

MODEL **V-P11L**

MODEL **V-P12**

Double bent tips. This tip is extra long to easily access difficult to reach areas and to avoid interference with neighbouring teeth or contours.

A longer version of the popular V-P10 tip.



ORDER CODE
Y1002165

- Pack of 3 • Right curved type*
- V10-S holder is not included



ORDER CODE
Y1002166

- Pack of 3 • Left curved type*
- V10-S holder is not included



V-P11R, V-P11L



ORDER CODE
Y1002167


- Pack of 3
- V10-S holder is not included



V-P12

■ V-P11R/L, V-P12 can be used only for VarioSurg 3 * The direction of the tip's curve is defined by the tip's anterior view.






ENDODONTICS

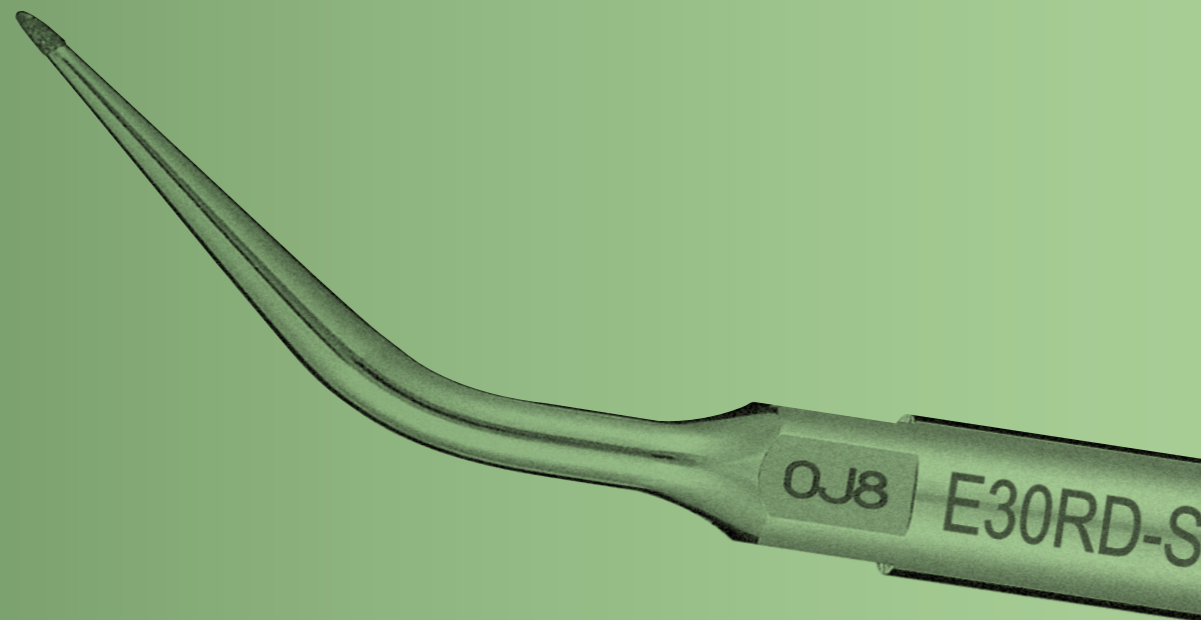

The microscopic diamond coated tip allows effective removal of dentin at the apex.

ENDODONTICS


MODEL **E30RD-S** POWERLEVEL ENDO 50% MODEL **E30LD-S** POWERLEVEL ENDO 50% MODEL **E31D-S** POWERLEVEL ENDO 50% MODEL **E32D-S** POWERLEVEL ENDO 50%



ORDER CODE

Z305118

- Diamond coating
- For posterior teeth (right angled*)



ORDER CODE

Z305119

- Diamond coating
- For posterior teeth (left angled*)



ORDER CODE

Z305120


- Diamond coating
- For anterior and posterior teeth (70°)




ORDER CODE

Z305121

- Diamond coating
- For anterior teeth (90°)



* The direction of the tip's angle is defined by the tip's anterior view.

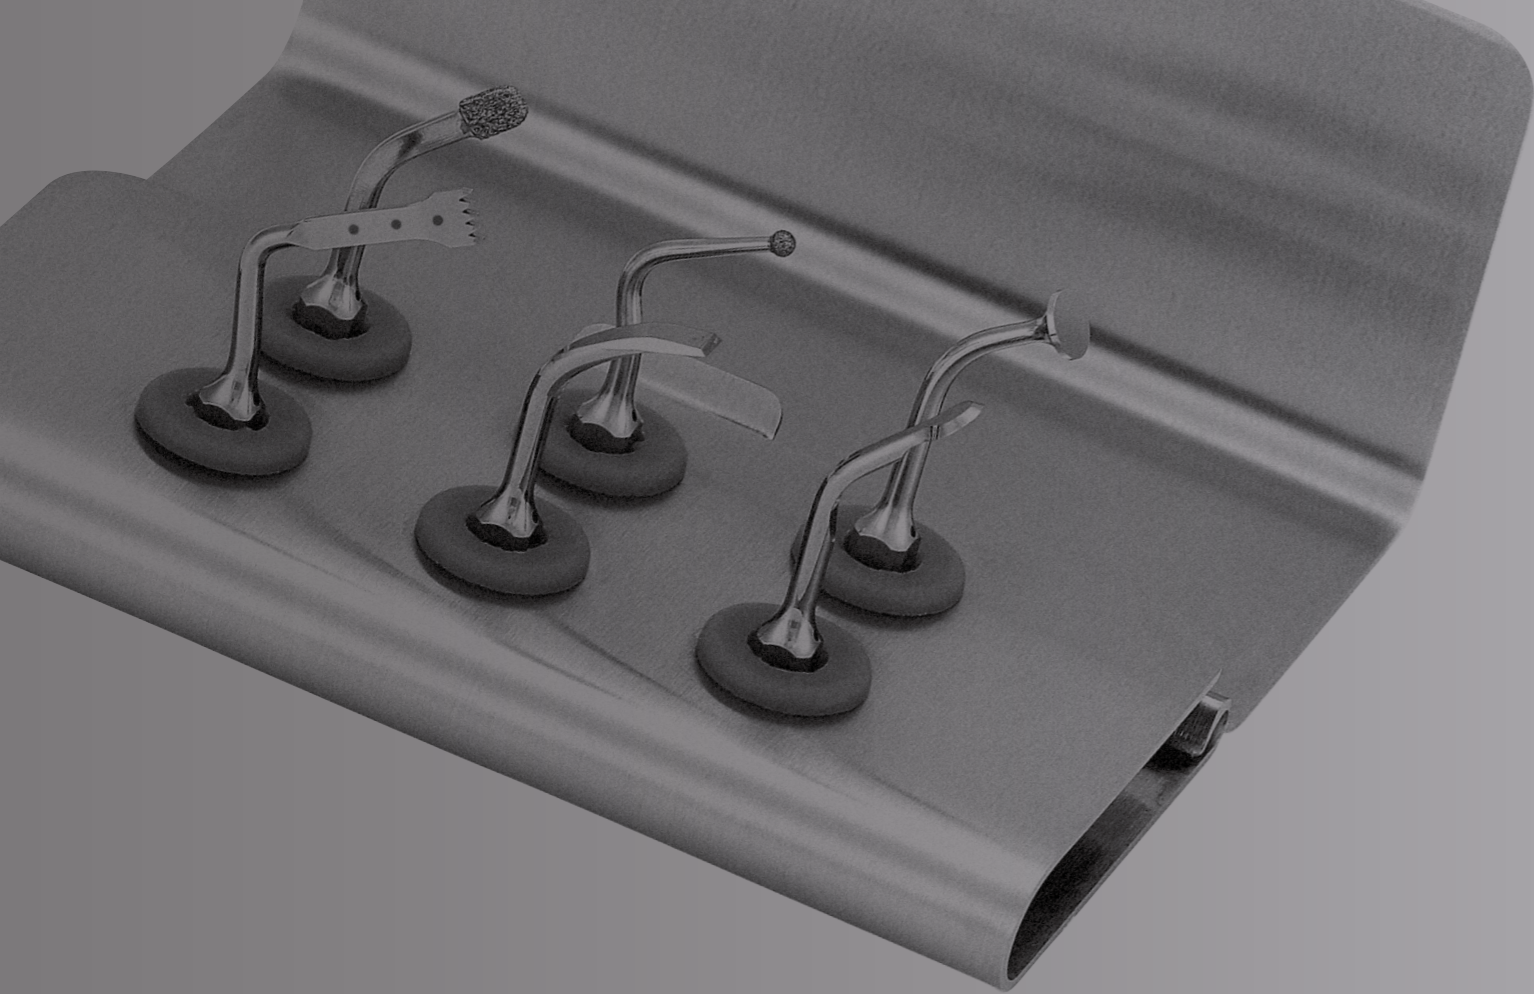

TIP KIT

TIP KIT

MODEL **Basic H-S Kit**

Contents

- H-SG1, SG3, SG5, SG6D, SG7D, SG11
- Tip holder



BONE SURGERY
SINUS LIFT
SCRAPER
SINUS MEMBRANE DETACHMENT

ORDER CODE

Y1002775

MODEL **Sinus Lift Kit**

Contents

- SG1, SG3, SG6D, SG9, SG10, SG11
- Tip holder



SINUS LIFT

ORDER CODE

Y900689

MODEL **Bone Cut Kit**

Contents

- SG1, SG2R, SG4, SG2L, SG6D
- Tip holder



BONE SURGERY

ORDER CODE

Y900688

MODEL **Endo-S Kit**

Contents

- G1-S, E30RD-S, E30LD-S, E31D-S, E32D-S
- Tip holder



ENDODONTICS

ORDER CODE

Y900691

MODEL **Implant Preparation Kit**

Contents

- SG15A, SG15B, SG16A, SG16B
- Tip holder



IMPLANT PREPARATION

ORDER CODE

Y900774

MODEL **Socket Lift (CRESTAL APPROACH) Kit for Wide Size Implant**

Contents

- SCL2D, SCL3D, SCL4D, SCL3
- VS Tip Wrench • Tip holder • Manual



SOCKET LIFT (CRESTAL APPROACH)

ORDER CODE

Y1002842

MODEL **Socket Lift (CRESTAL APPROACH) Kit for Regular Size Implant**

Contents

- SCL1D, SCL2D, SCL1
- VS Tip Wrench • Tip holder • Manual



SOCKET LIFT (CRESTAL APPROACH)

ORDER CODE

Y1002841

VarioSurg 4

Advantages

- Super slim handpiece with LED
- Extensive tip range for a wide range of applications
- Link 2 system with Surgic Pro2 (implant motor)



Complete Set

Optic	MODEL	ORDER CODE
●	VarioSurg 4 (230V)	Y1500706

Contents

- Control Unit • LED Handpiece with 2m cord • FC-86 Foot Control
- Sterilization Cassette • Handpiece Stand
- Irrigation tube (3 pcs.) and other accessories
- Basic H-S Kit (H-SG1, SG3, SG5, SG6D, SG7D, SG11 and Tip holder)

Complete Set without Foot Control

Optic	MODEL	ORDER CODE
●	VarioSurg 4 w/o FC (230V)	Y1500712

Contents

- Control Unit • LED Handpiece with 2m cord • Sterilization Cassette
- Handpiece Stand • Irrigation tube (3 pcs.) and other accessories
- Basic H-S Kit (H-SG1, SG3, SG5, SG6D, SG7D, SG11 and Tip holder)

Specifications (Control Unit)

- Frequency : 28-32 kHz
- Power Supply : AC100 - 240V 50/60 Hz
- Max. Pump Output : 76 mL / min
- Programs : SURG x 5, ENDO x 2, PERIO x 2
- Dimensions : W 245 x D 235 x H 90 mm

NAKANISHI INC. www.nsk-dental.com
700 Shimohinata, Kanuma, Tochigi 322-8666, Japan

NSK Europe GmbH
Elly-Beinhorn-Str. 8
65760 Eschborn
Germany

NSK United Kingdom Ltd.
Office 4, Gateway 1000
Arlington Business Park
Whittle Way, Stevenage
SG1 2FP, UK

NSK Dental Nordic
Furstenbergsgatan 4
416 64 Gothenburg
Sweden

Specifications are subject to change without notice.